LS AFM – Stage

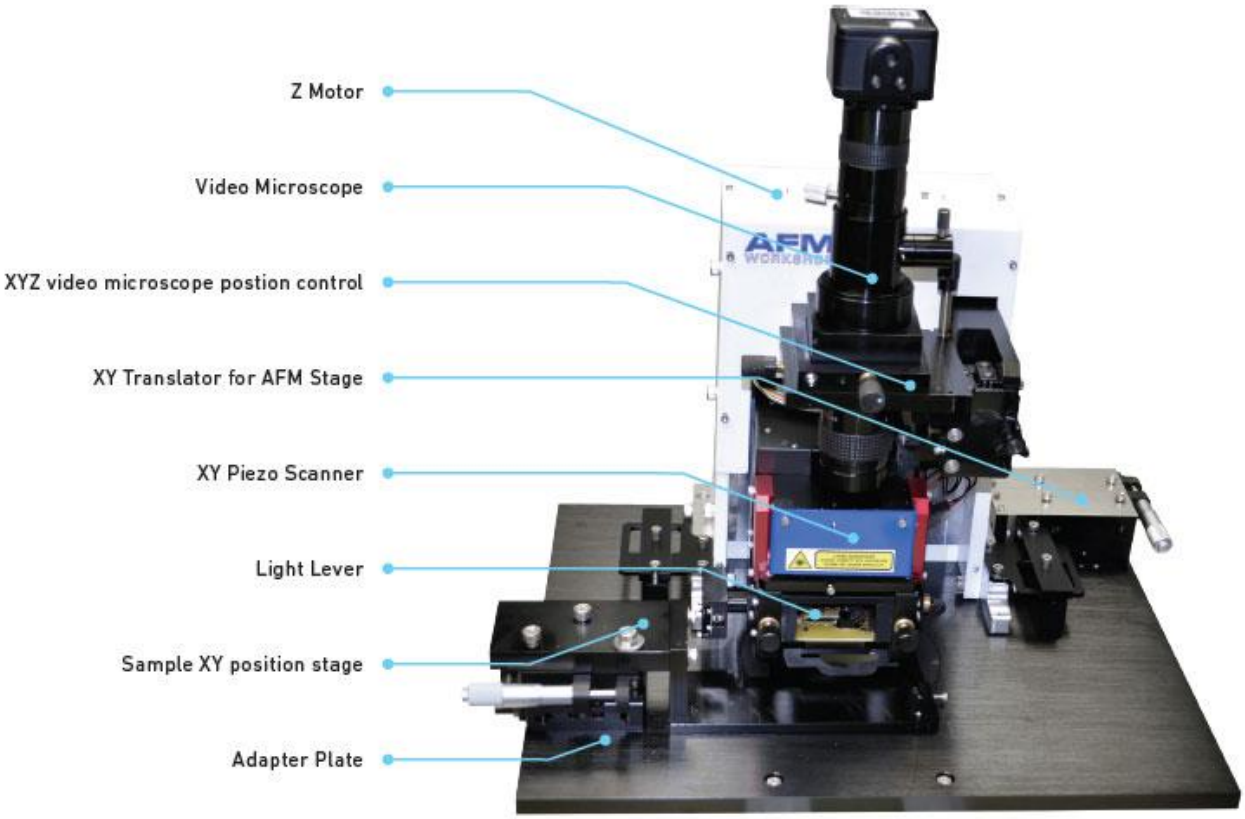

AFM STAGE

The AFM Stage is secured on an adapter plate that is attached to the inverted optical microscope. There is an XY translation stage for moving the sample under the AFM Probe. Additionally there is an XY translation stage for moving the AFM over the inverted optical microscope axis.

▶ Sample Stage for the LS-AFM

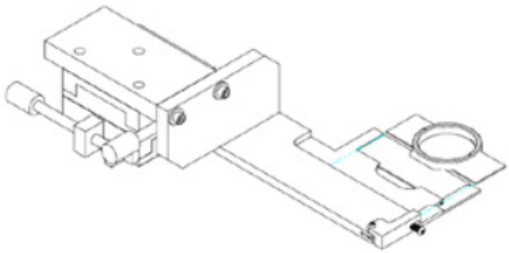
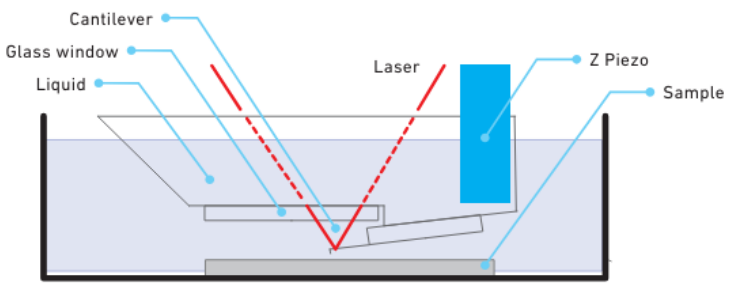
▶ Z Scanner for Liquid Imaging